

CERTIFICATE OF ANALYSIS

Product Name	(Gly14)-Humanin Cat.#: 312862 (TFA removed)
Lot No.	MTFA30864-1228
Sequence	MAPRGFSCLLLLTGEIDL PVKRRRA (Acetate Salt)
Dissolution condition	15%ACN+85%H ₂ O
Length	24AA
Modification	acetate salt
Molecular Weight (MW)	2657.18
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2657.25	Conforms
Purity by HPLC	>95%	95.827%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	40mg	5.0mg*8

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Jan/16/2024




Sample Information

Order ID :MTFA30864
 Name :(Gly14)-Humanin
 Sequence :MAPRGFSCLLLLTGEIDLPKRRA (Acetate Salt)
 Lot. No :MTFA30864-1228
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Phenomenex Luna® 5 µm C18 (2) (4.6*250mm*5 µm)
 Dissolution method :15%ACN+85%H2O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	35
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	35
50.00	Controller	Stop	

Chromatogram

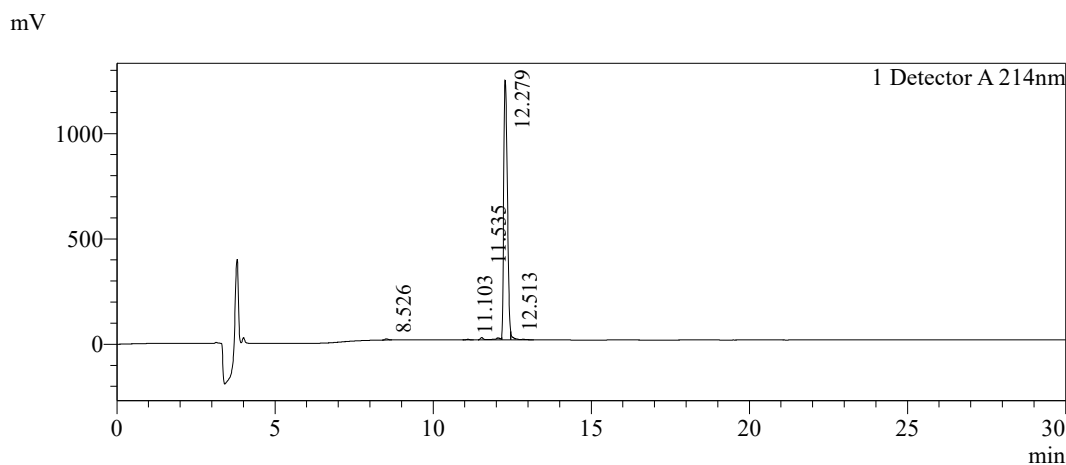


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	8.526	41446	5624	0.397
2	11.103	20646	2818	0.198
3	11.535	188952	10948	1.809
4	12.279	10010185	1232219	95.827
5	12.513	184925	13160	1.770
Total		10446153	1264770	100.000

MS Spectrum

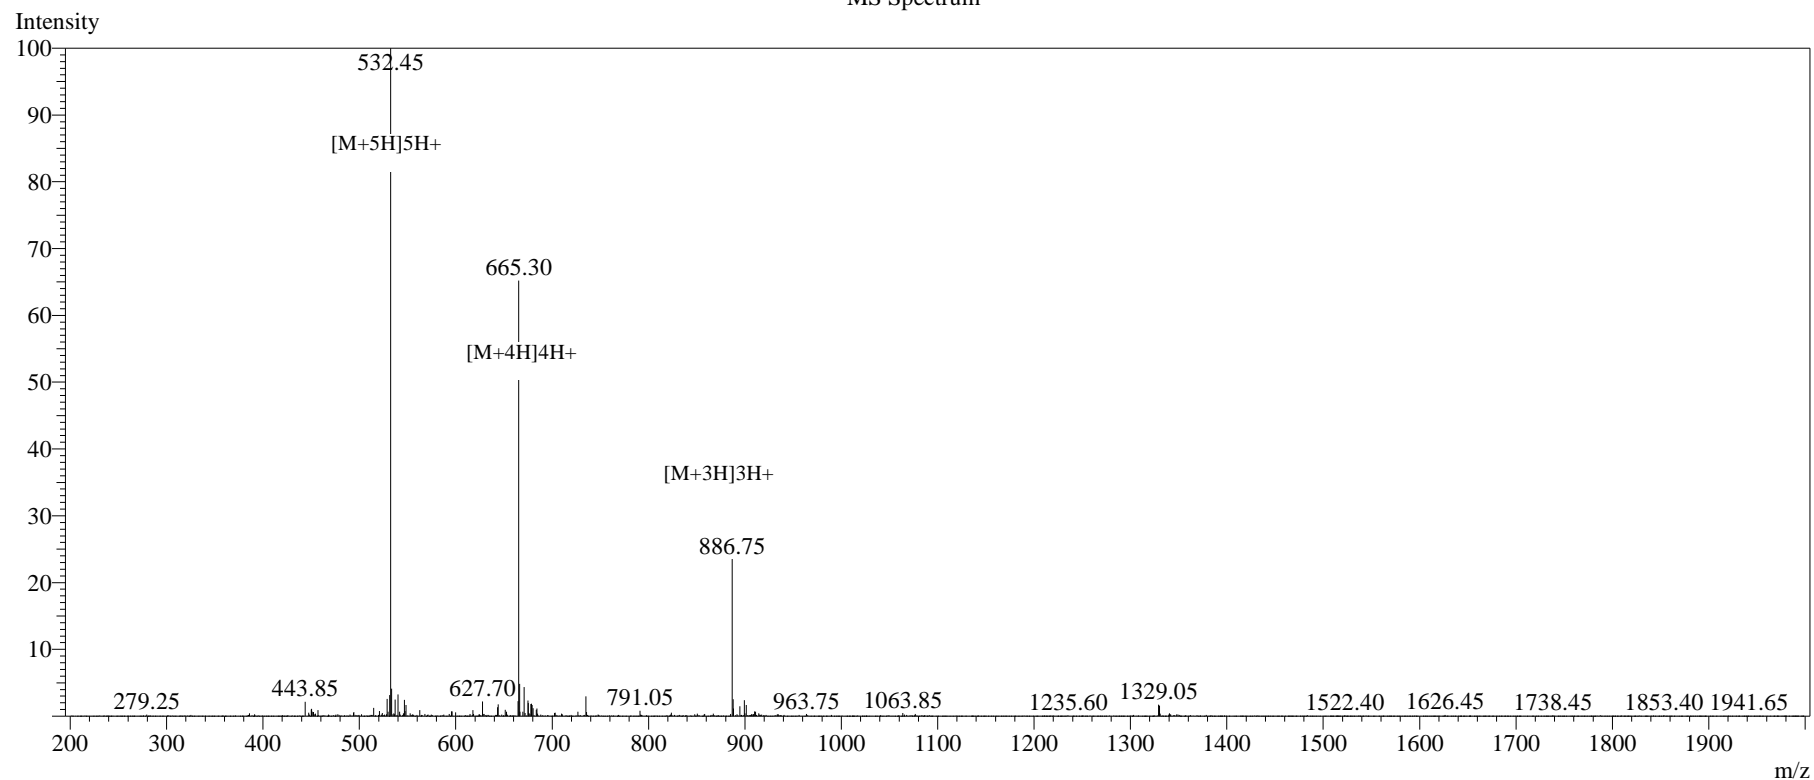

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/01/11 15:00:56	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA30864
Name	:(Gly14)-Humanin
Sequence	:MAPRGFSCLLLLTGEIDL PVKRRRA(Acetate Salt)
Lot.No	:MTFA30864-1228
Theoretical	:2657.18
Observed	:2657.25