

CERTIFICATE OF ANALYSIS

Product Name	Biotin-FLAG peptide, Cat.#: 319196 (TFA removed)
Lot No.	MTFA31136-0320
Sequence	Biotin-DYKDDDDK (Acetate Salt)
Dissolution condition	2%NH3.H2O+18%ACN+80%H2O
Length	8AA
Modification	Acetate salts
Molecular Weight (MW)	1239.26
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1239.00	Conforms
Purity by HPLC	>95%	96.950%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	50mg	5.0mg*10

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Mar/26/2024




Sample Information

Order ID :MTFA31136
 Name :Biotin-FLAG peptide
 Sequence :Biotin-DYKDDDDK (Acetate Salt)
 Lot. No :MTFA31136-0320
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Phenomenex Luna® 5 µm C18(2) (4.6*250mm*5 µm)
 Dissolution method :2%NH3.H2O+18%ACN+80%H2O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	5
30.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	5
50.00	Controller	Stop	


Chromatogram

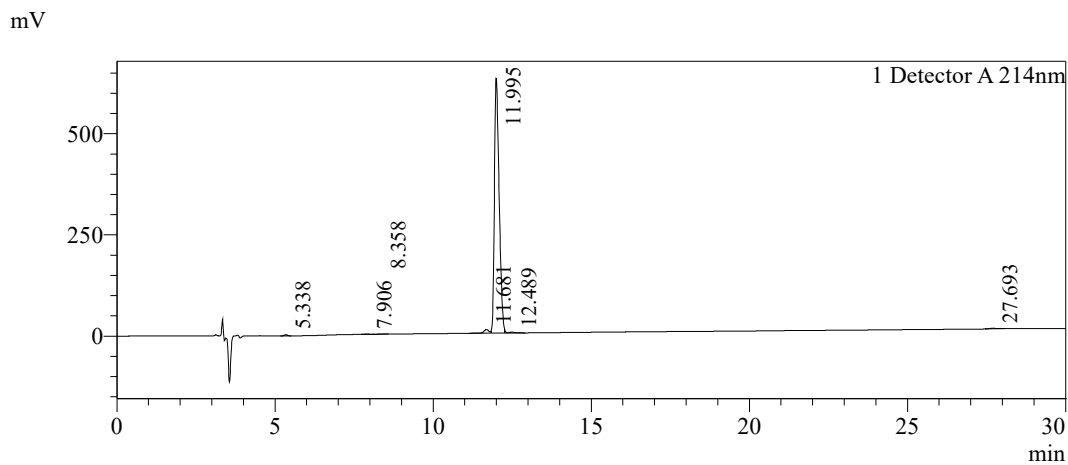

Peak Table

Detector A 214nm				
Peak#	Ret. Time	Area	Height	Area%
1	5.338	17386	2729	0.256
2	7.906	5421	549	0.080
3	8.358	2635	294	0.039
4	11.681	112339	9262	1.656
5	11.995	6575553	629504	96.950
6	12.489	43775	2125	0.645
7	27.693	25319	1310	0.373
Total		6782427	645771	100.000

MS Spectrum

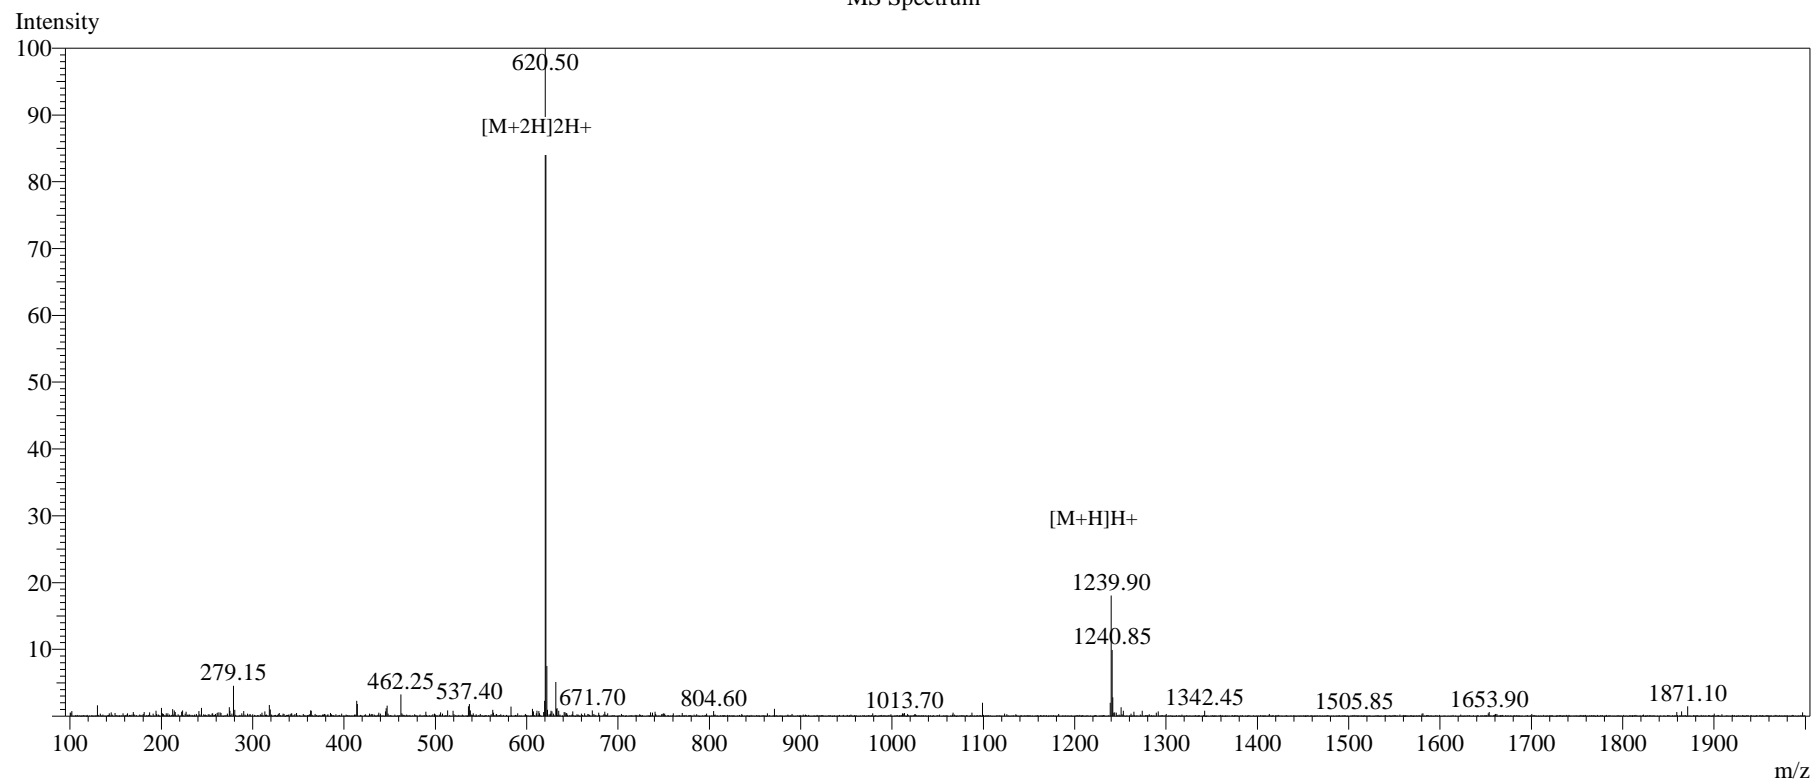

Sample Information

Dissolution method	:2%NH ₃ .H ₂ O+18%ACN+80%H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/03/25 11:56:03	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H ₂ O/50%MEOH

Order ID	:MTFA31136
Name	:Biotin-FLAG peptide
Sequence	:Biotin-DYKDDDDK (Acetate Salt)
Lot.No	:MTFA31136-0320
Theoretical	:1239.26
Observed	:1239.00