

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	Buforin I Cat.# 305785
<b>Lot No.</b>	GT30919-1123
<b>Sequence</b>	AGRKGQGGKVRAKAKTRSSRAGLQFPVGRVHLLLRKGNV
<b>Dissolution condition</b>	100%H <sub>2</sub> O
<b>Length</b>	39AA
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	4262.94
<b>Storage</b>	-20°C

---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	4263.85	Conforms
<b>Purity by HPLC</b>	>98%	98.262%
<b>Peptide Content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	40mg	40.0mg

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Jan/19/2018




Sample Information

Order ID :GT30919  
 Name :N/A  
 Sequence :AGRGKQGGKVRAKAKTRSSRAGLQFPVGRVHLLLRKGN  
 Lot. No :GT30919-1123  
 Pump A :0.1% Trifluoroacetic in 100% water  
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :SHIMADZU Inertsil ODS-SP(4.6\*250mm\*5um)  
 Dissolution method :100% H2O  
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	2
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	2
50.00	Controller	Stop	

Chromatogram

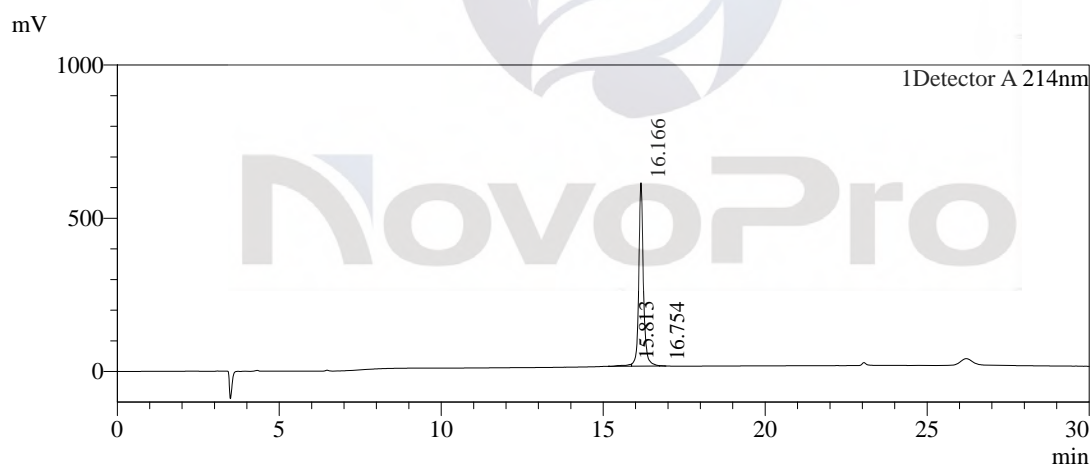


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	15.813	99025	5040	1.648
2	16.166	5903310	598146	98.262
3	16.754	5401	902	0.090
Total		6007735	604087	100.000

# MS Spectrum

Positive Intensity

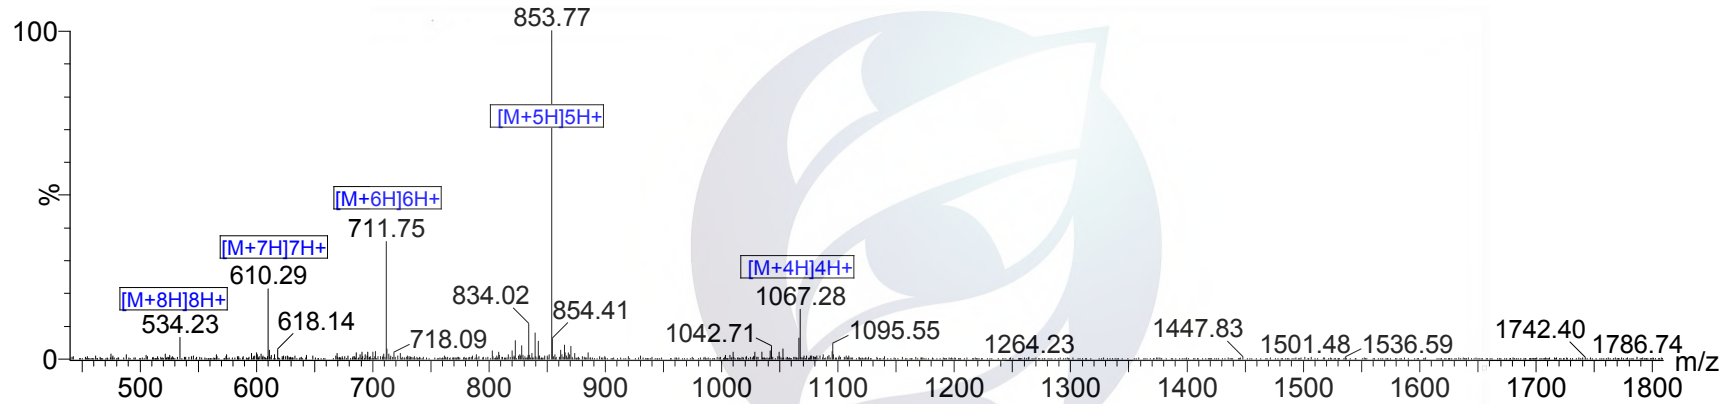

Dissolution method	: 5% HAC + 8% ACN + 87% H <sub>2</sub> O	Interface	: ESI	Prerod Bias	: +4.5kv
Date Acquired	: 2018/1/18 9:37:25	Nebulizing Gas Flow	: 1.50L/min	Detector	: -0.2kv
Injection Volume	: 0.2ul	CDL Temp	: 250C	T.Flow	: 0.2ml/min
Block Temp	: 200	CDL Volt	: 0v	B.conc	: 50% H <sub>2</sub> O / 50% MEOH

Order ID	: GT30919
Name	: N/A
Sequence	: AGRGKQGKVRRAKAKTRSSRAGLQFPVGRVHRLLRKGNV
Lot.No	: GT30919-1123
Theoretical	: 4262.94
Observed	: 4263.85

