

## CERTIFICATE OF ANALYSIS

Product Name	DRGN-1 peptide, Cat.#: 318919 (TFA removed)
Lot No.	MTFA32805-250512
Sequence	PSKKTKPVKPKKVA (Acetate Salt)
Dissolution condition	100%H <sub>2</sub> O
Length	14AA
Modification	acetate salt
Molecular Weight (MW)	1535.92
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1536.00	Conforms
Purity by HPLC	>95%	95.070%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	100mg	5.0mg*20

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



May/15/2025


Quality Assurance Department



### Sample Information

Order ID	:MTFA32805		
Name	:DRGN-1 peptide (TFA removed)		
Sequence	:PSKKTKPVKPKKVA (Acetate Salt)		
Lot. No	:MTFA32805-250512		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	5
30.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	5
50.00	Controller	Stop	

### Chromatogram

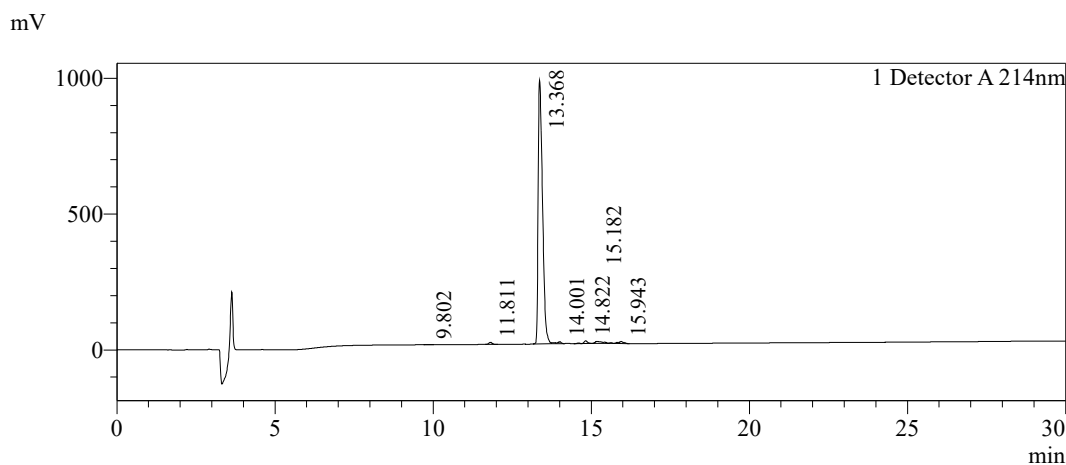


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	9.802	7250	887	0.074
2	11.811	55879	7888	0.571
3	13.368	9298924	970055	95.070
4	14.001	75403	6476	0.771
5	14.822	98217	10294	1.004
6	15.182	153325	7781	1.568
7	15.943	92098	7522	0.942
Total		9781095	1010903	100.000

# MS Spectrum

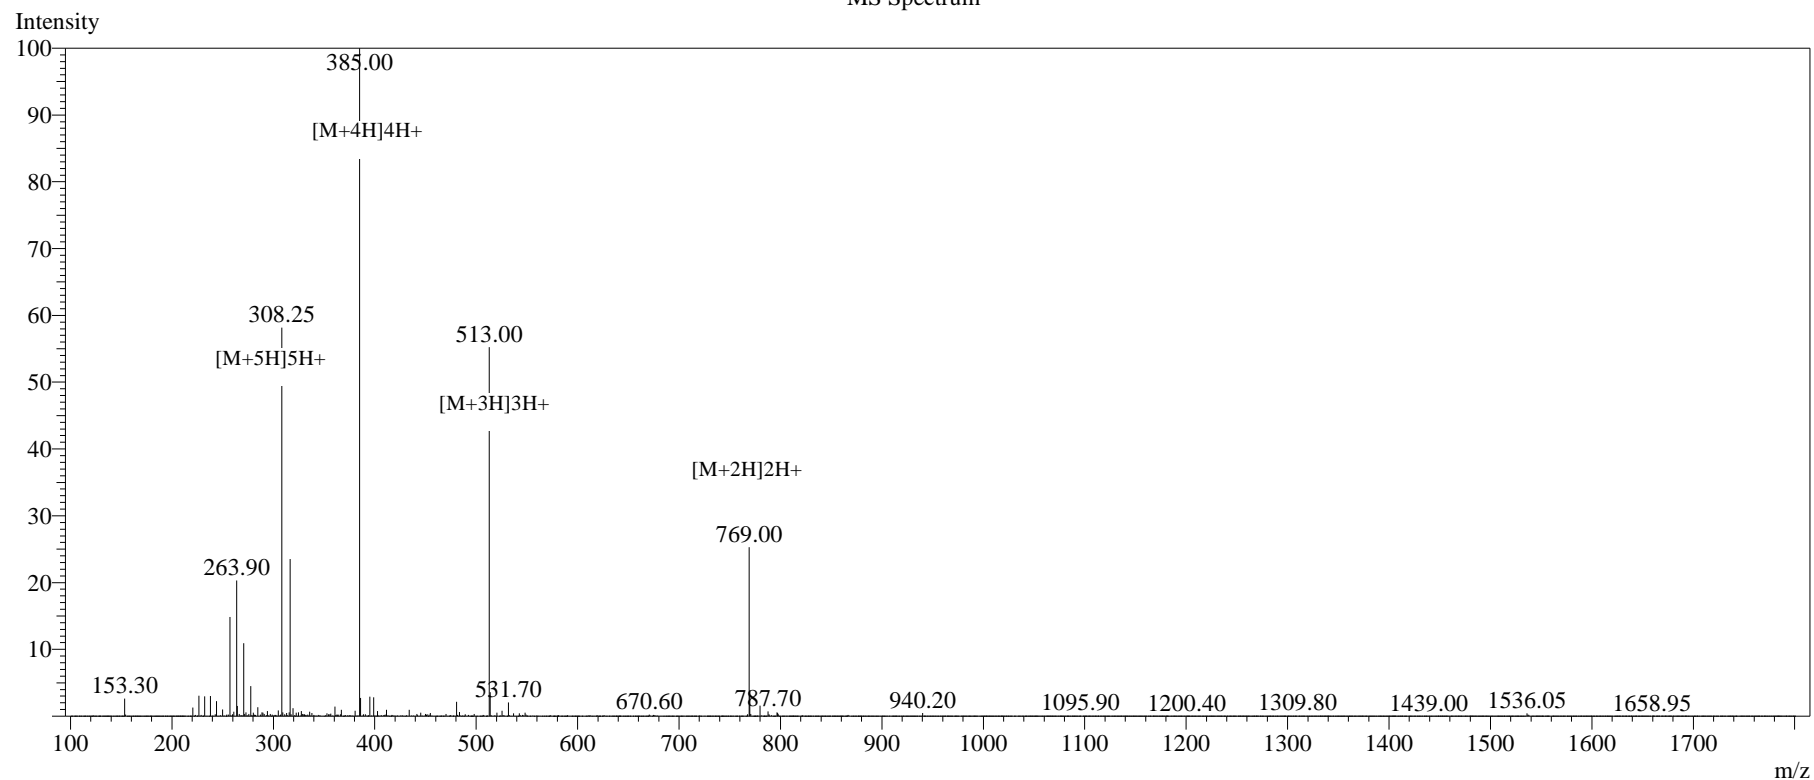

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/05/14 14:37:47	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% ME OH

Order ID	:MTFA32805
Name	:DRGN-1 peptide (TFA removed)
Sequence	:PSKKTKPVKPKKVA (Acetate Salt)
Lot.No	:MTFA32805-250512
Theoretical	:1535.92
Observed	:1536.00