

CERTIFICATE OF ANALYSIS

Product Name	MBP(111-129) peptide, Cat.#: 319175
Lot No.	MTFA32630-0403
Sequence	LSRFSWGAEGQRPFGYGG
Dissolution condition	15%ACN+85%H2O
Length	19AA
Modification	N/A
Molecular Weight (MW)	2029.18
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2029.20	Conforms
Purity by HPLC	>95%	96.821%
TFA content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Apr/08/2025


Quality Assurance Department



Sample Information

Order ID	:MTFA32630		
Name	:MBP(111-129) peptide		
Sequence	:LSRFSWGAEGQRPGFGYGG		
Lot. No	:MTFA32630-0403		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:15%ACN+85%H2O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	


Chromatogram

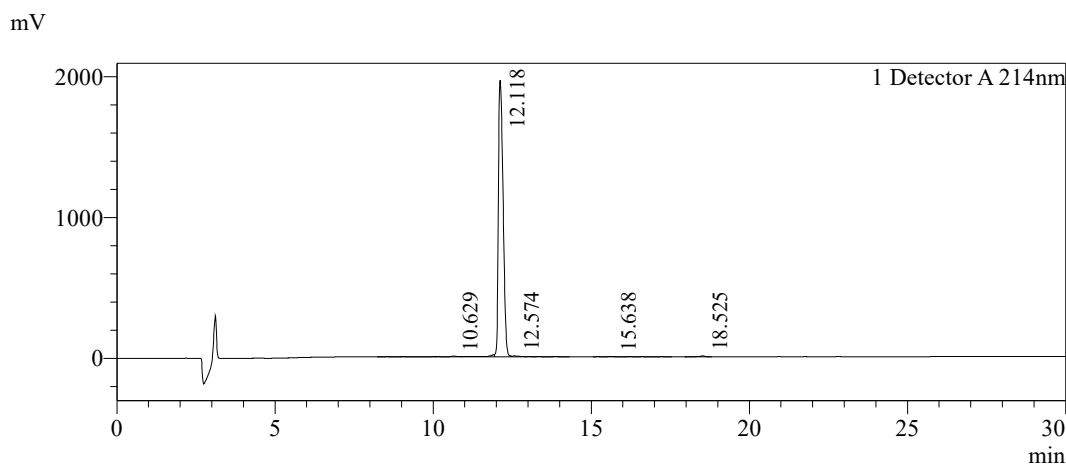

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.629	387823	5275	1.847
2	12.118	20335039	1962840	96.821
3	12.574	148263	5771	0.706
4	15.638	69991	2501	0.333
5	18.525	61679	5682	0.294
Total		21002796	1982069	100.000

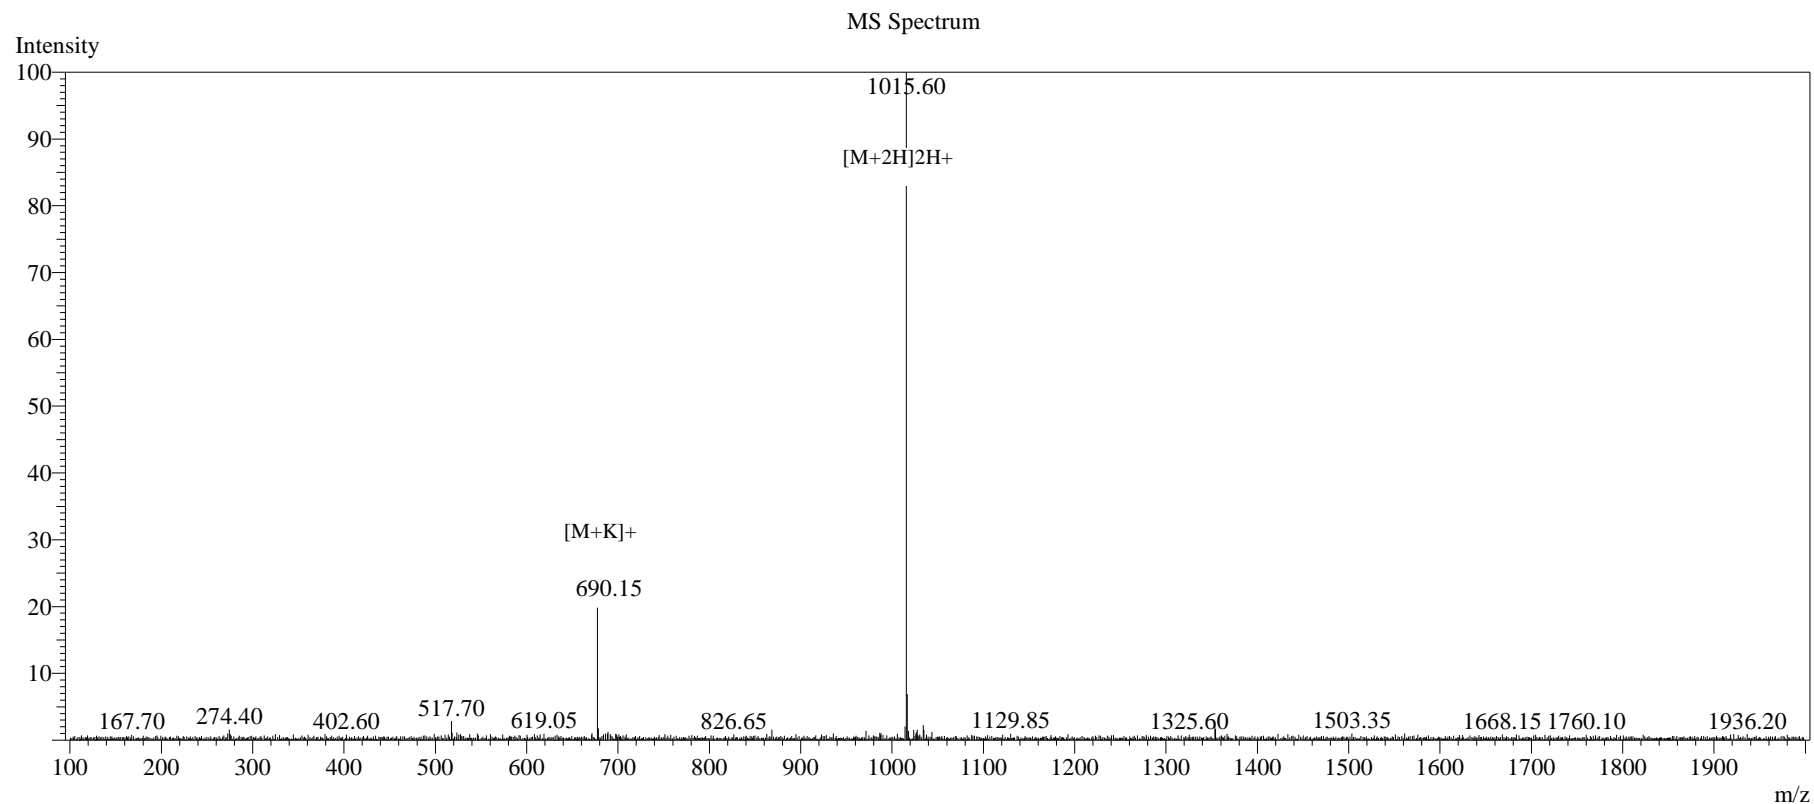

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/04/07 13:47:14	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% ME OH

Order ID	:MTFA32630
Name	:MBP(111-129) peptide
Sequence	:LSRFSWGAEGQRPFGYGG
Lot.No	:MTFA32630-0403
Theoretical	:2029.18
Observed	:2029.20