

CERTIFICATE OF ANALYSIS

Product Name	Oncl12 peptide
Lot No.	GTA32861-0707
Sequence	VDKPPYLPRPRPPRrIYNr-NH2
Dissolution condition	100%H2O
Length	19AA
Modification	r=D-Arg
Molecular Weight (MW)	2389.79
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2390.10	Conforms
Purity by HPLC	>95%	95.444%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	100mg	5.0mg*20

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

July/07/2020




Sample Information

Order ID :GTA32861
 Name :Onc112 peptide
 Sequence :VDKPPYLPRPRPPRrIYNr-NH2
 Lot. No :GTA32861-0707
 Pump A :0.1% Trifluoroacetic in 100% water
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :SHIMADZU Inertsil ODS-SP(4.6*250mm*5um)
 Dissolution method :100% H2O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	15
20.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

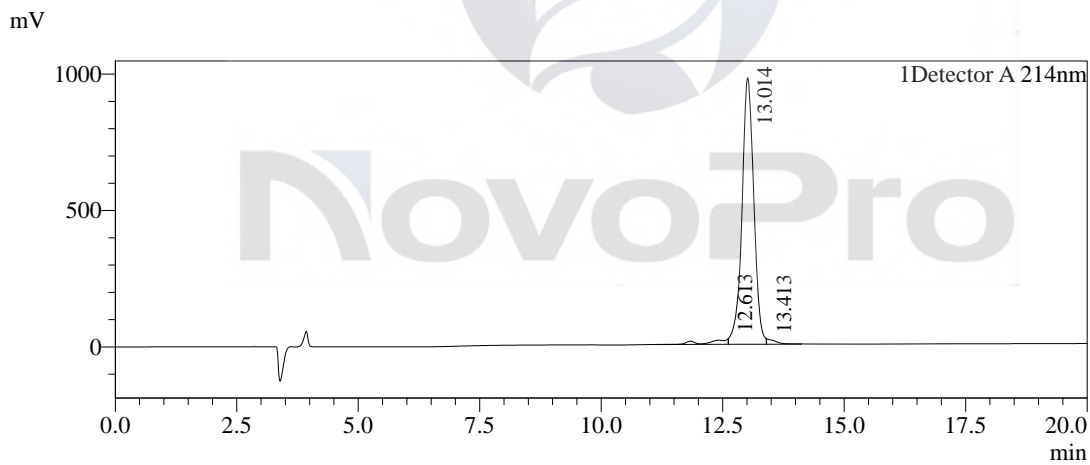


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.613	545126	19712	3.142
2	13.014	16559363	976475	95.444
3	13.413	245397	19791	1.414
Total		17349886	1015978	100.000

MS Spectrum

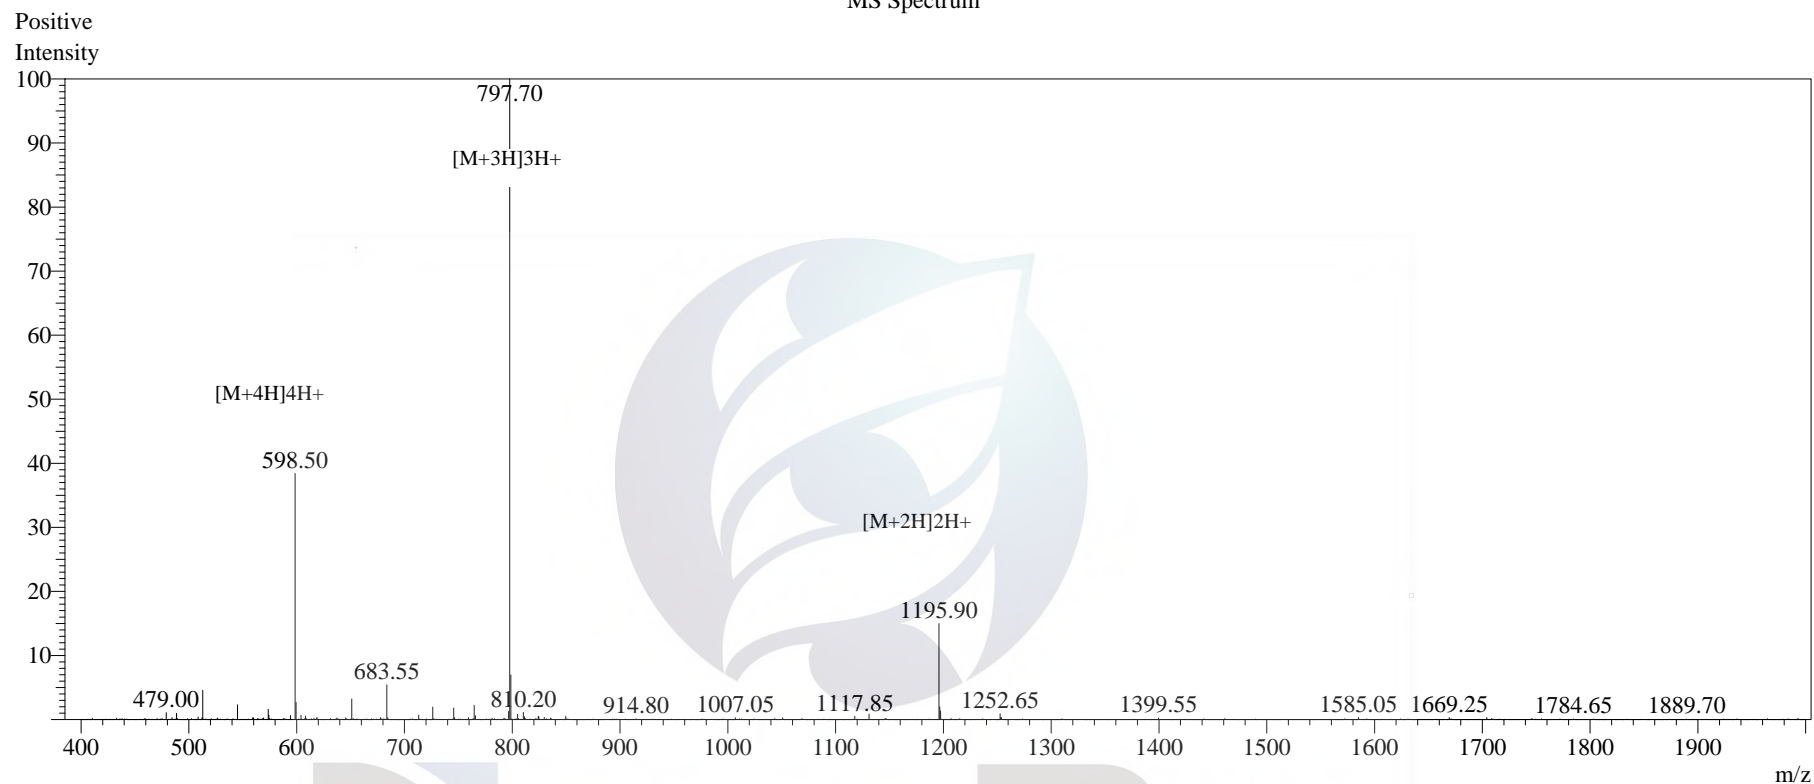

Sample Information

Dissolution method	:5% HAC+8% ACN+87% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2020/07/15 16:19:35	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:GTA32861
Name	:Onc112 peptide
Sequence	:VDKPPYLPRPRPPRrIYNr-NH ₂
Lot.No	:GTA32861-0707
Theoretical	:2389.79
Observed	:2390.10