

## CERTIFICATE OF ANALYSIS

Product Name	Preprocaerulein I precursor [34-43], Cat.#: 308850
Lot No.	MTFA32955-01-250618
Sequence	GLASFLGKAL
Dissolution condition	100%H <sub>2</sub> O
Length	10AA
Modification	N/A
Molecular Weight (MW)	976.15
Storage	-20°C

Test Items	Specifications	Results
MW by MS	976.20	Conforms
Purity by HPLC	>95%	99.502%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20 mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Jul/08/2025


Quality Assurance Department



### Sample Information

Order ID	:MTFA32955-01		
Name	:Preprocaerulein I precursor [34-43]		
Sequence	:GLASFLGKAL		
Lot. No	:MTFA32955-01-250618		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H <sub>2</sub> O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

### Chromatogram

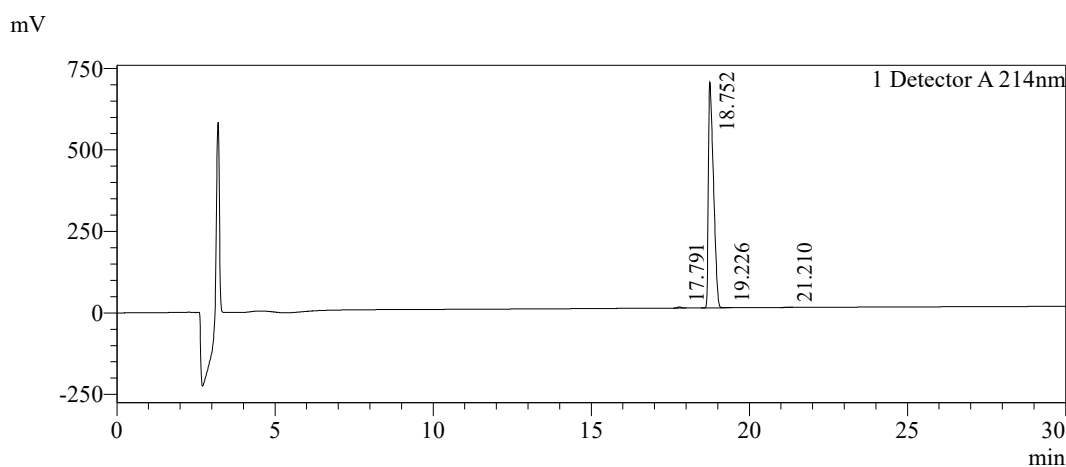


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	17.791	27157	3632	0.347
2	18.752	7784890	691820	99.502
3	19.226	8249	789	0.105
4	21.210	3595	465	0.046
Total		7823892	696706	100.000

# MS Spectrum

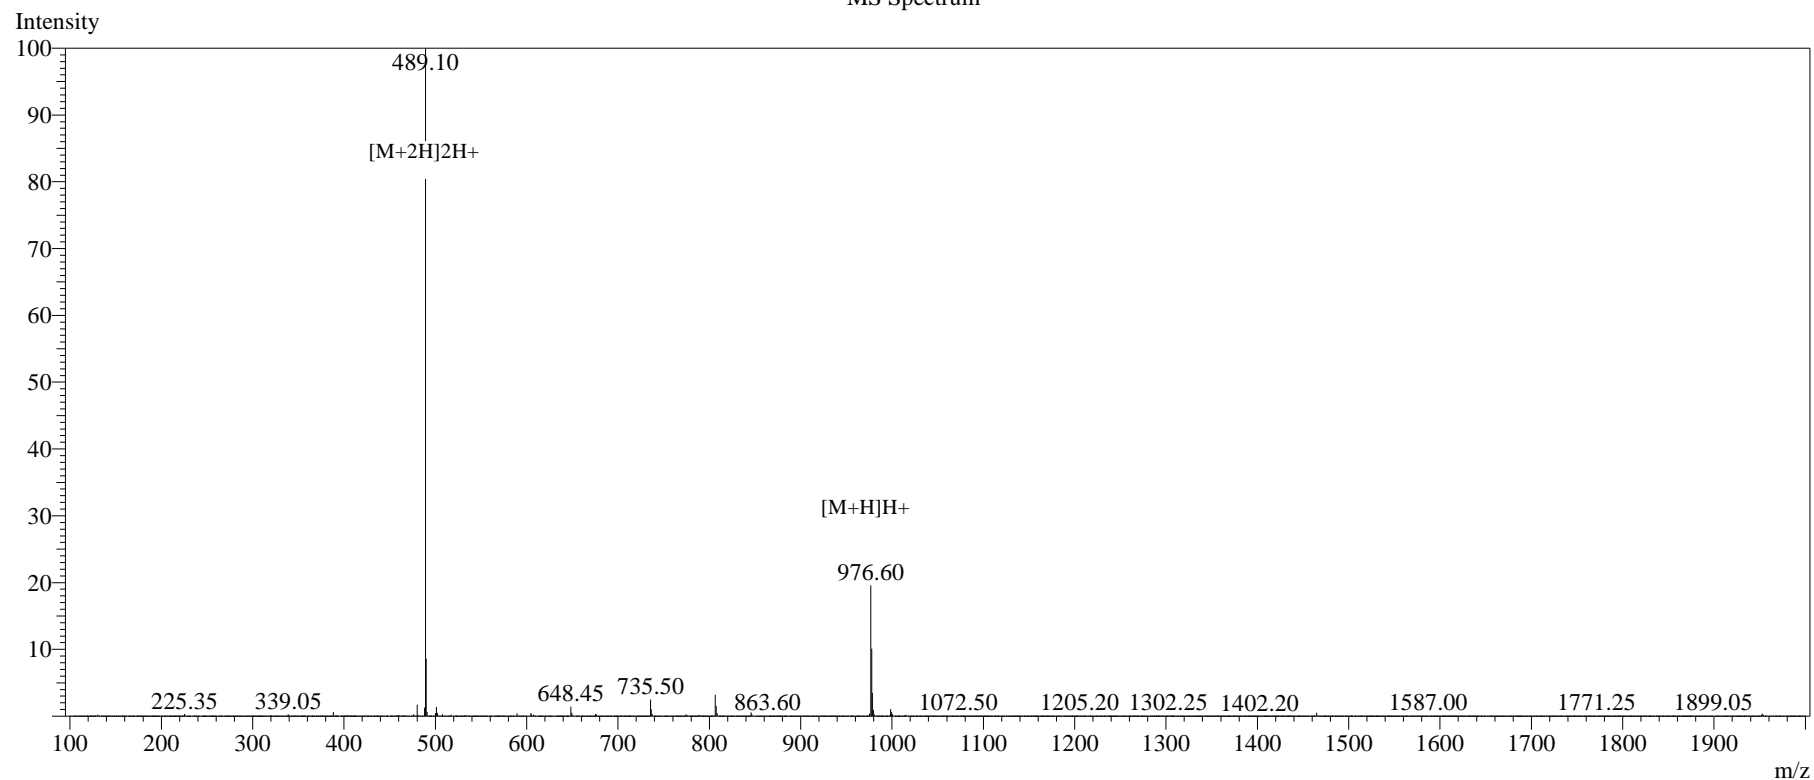

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/07/02 10:57:19	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% ME OH
Order ID	:MTFA32955-01				
Name	:Preprocaerulein I precursor [34-43]				
Sequence	:GLASFLGKAL				
Lot.No	:MTFA32955-01-250618				
Theoretical	:976.15				
Observed	:976.20				