

CERTIFICATE OF ANALYSIS

Product Name	Rattin [1-24] peptide, Cat.#:302311
Lot No.	MTFA30069-0403
Sequence	MAKRGFNCLLLSISEIDLVPKRLE-NH2
Dissolution condition	100%H2O
Length	24AA
Modification	N/A
Molecular Weight (MW)	2745.29
Storage	-20°C

Test Items	Specifications	Results
MW by MS	2745.39	Conforms
Purity by HPLC	95.0%	96.904%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	100mg	5.0mg*20

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Apr/25/2023




Sample Information

Order ID :MTFA30069
 Name :Rattin 1-24 peptide
 Sequence :MAKRGFNCLLLSISEIDLPKRLE-NH2
 Lot. No :MTFA30069-0403
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Shim-pack GIST C18(4.6*250mm*5um)
 Dissolution method :100%H2O
 Inj. Volume : 20ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	25
20.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	25
50.00	Controller	Stop	

Chromatogram

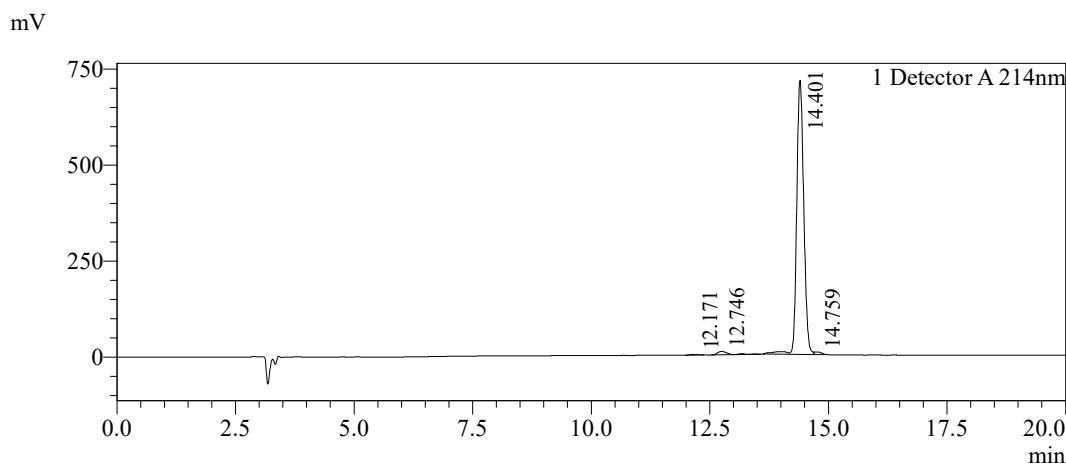


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	12.171	16752	1568	0.219
2	12.746	151748	8918	1.987
3	14.401	7401844	713763	96.904
4	14.759	67992	6447	0.890
Total		7638336	730695	100.000

MS Spectrum

Positive
Intensity

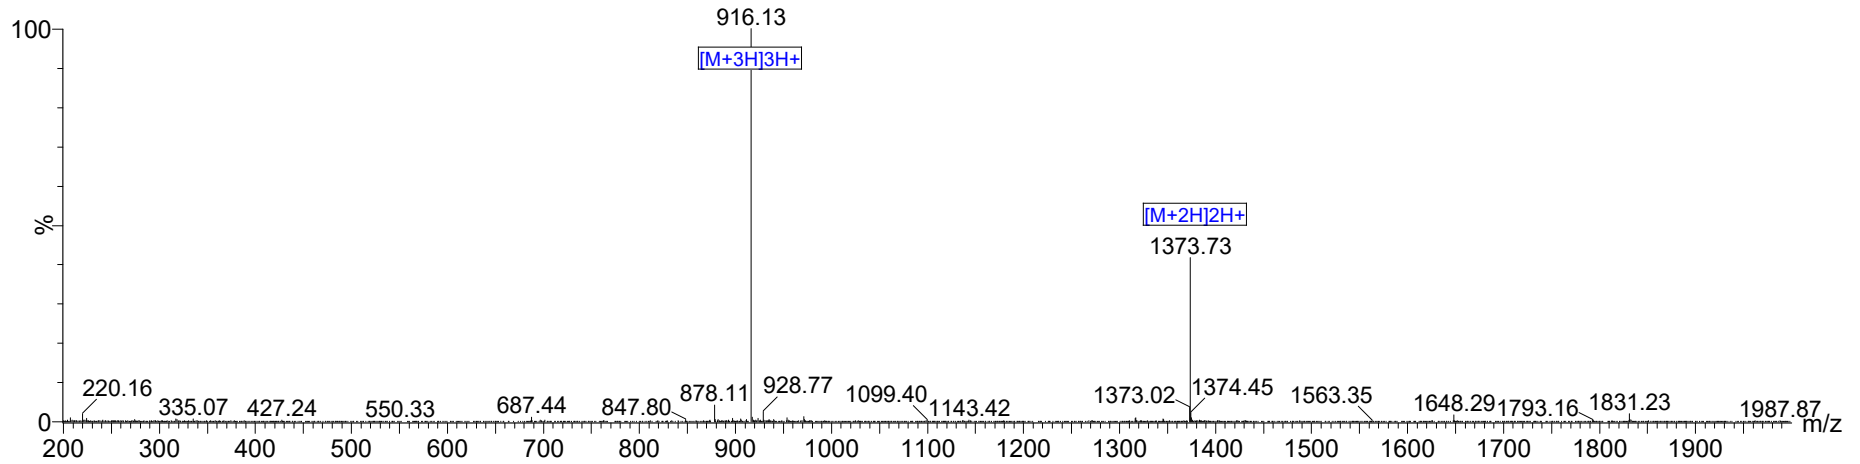

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2023/3/13 9:36:24	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID : MTF30069
 Name : Rattin 1-24 peptide
 Sequence : MAKRGFNCLLLSISEIDLPKRLE-NH2
 Lot.No : MTF30069-0403
 Theoretical : 2745.29
 Observed : 2745.39