

## CERTIFICATE OF ANALYSIS

Product Name	SIFamide, Cat.#: 318512 (TFA removed)
Lot No.	MTFA32771-1-0430
Sequence	TRKLPFNGSIF-NH2 (Acetate Salt)
Dissolution condition	100%H2O
Length	11AA
Modification	acetate salt
Molecular Weight (MW)	1278.50
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1278.50	Conforms
Purity by HPLC	>95%	99.461%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



May/22/2025

Quality Assurance Department




### Sample Information

Order ID	:MTFA32771-1		
Name	:SIFamide		
Sequence	:TRKLPGNGSIF-NH2 (Acetate Salt)		
Lot. No	:MTFA32771-1-0430		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

### Chromatogram

mV

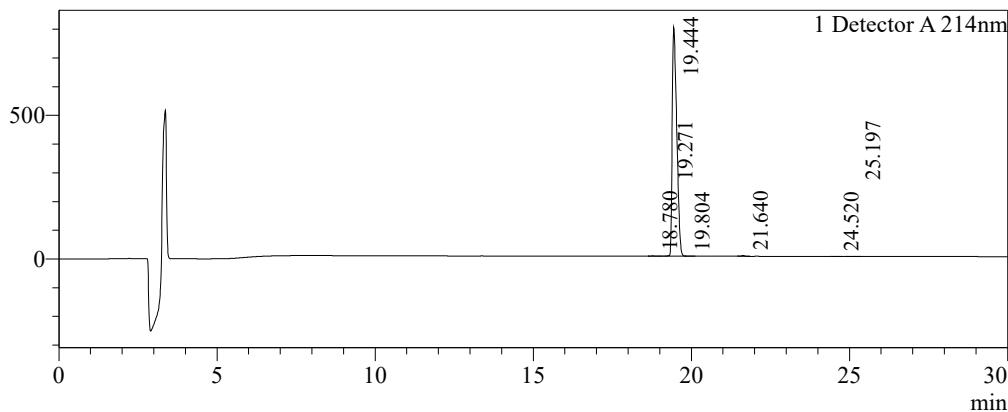


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	18.780	9678	821	0.121
2	19.271	4326	1122	0.054
3	19.444	7972369	796927	99.461
4	19.804	4282	640	0.053
5	21.640	18894	2546	0.236
6	24.520	1295	146	0.016
7	25.197	4711	409	0.059
Total		8015555	802611	100.000

# MS Spectrum

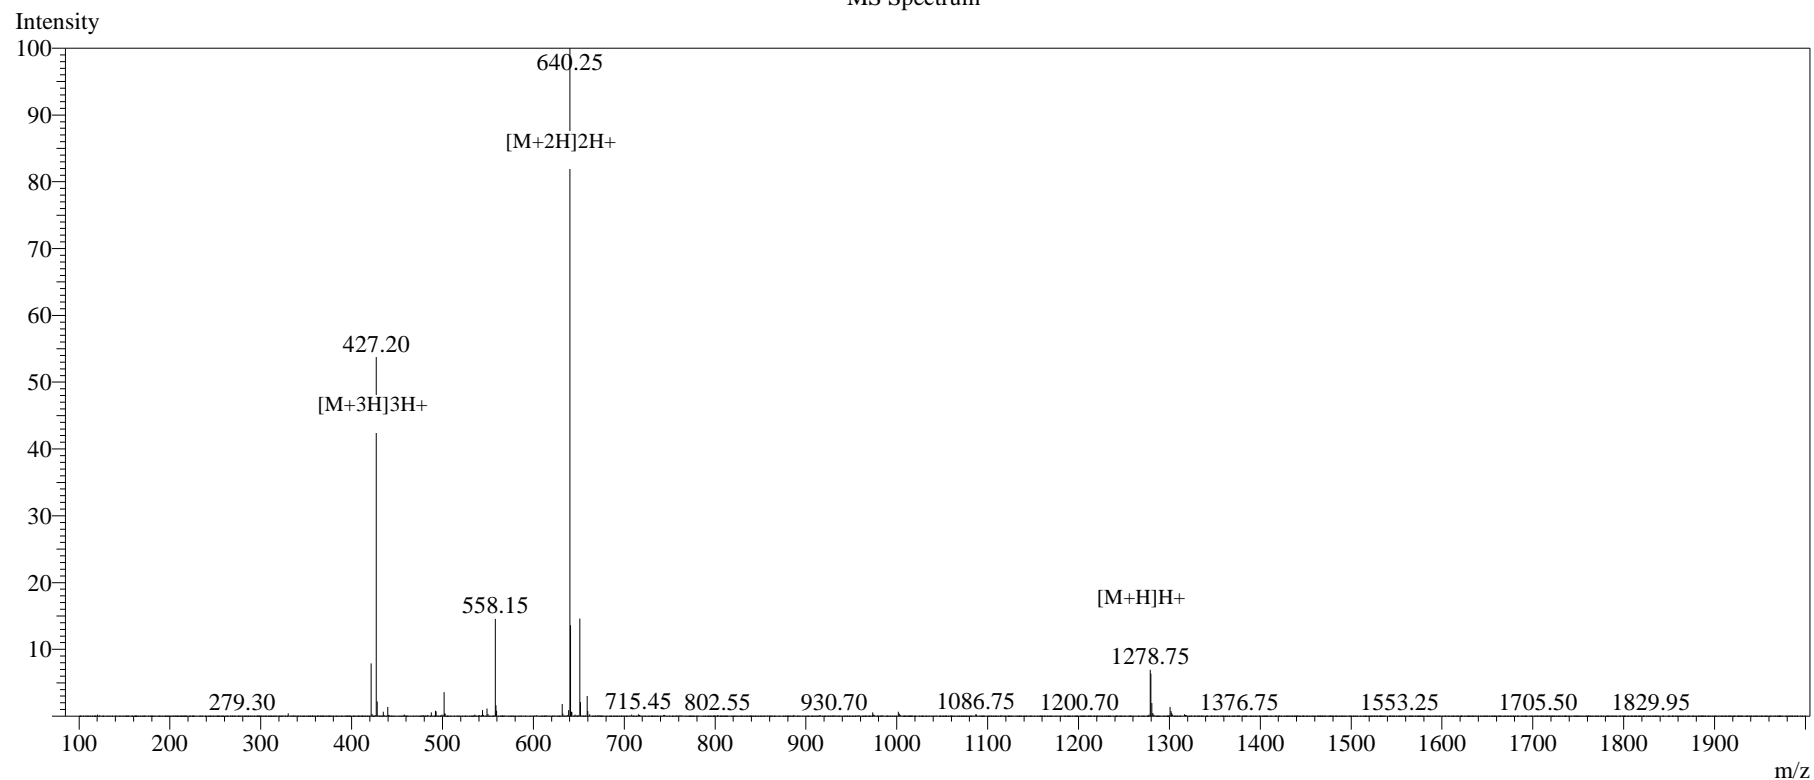

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/05/15 13:28:16	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% ME OH
Order ID	:MTFA32771-1				
Name	:SIFamide				
Sequence	:TRKLPFNGSIF-NH <sub>2</sub> (Acetate Salt)				
Lot.No	:MTFA32771-1-0430				
Theoretical	:1278.50				
Observed	:1278.50				