

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	Tat-CIRP peptide, Cat.#: 319097
<b>Lot No.</b>	MTFA30261-0705
<b>Sequence</b>	YGRKKRRQRRRGRGFSRGGGDRGYGG
<b>Dissolution condition</b>	100%H <sub>2</sub> O
<b>Length</b>	26AA
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	2997.32
<b>Storage</b>	-20°C

---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	2996.64	Conforms
<b>Purity by HPLC</b>	>95%	98.470%
<b>Peptide Content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	20mg	5.0mg*4

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

July/24/2023




### Sample Information

Order ID :MTFA30261  
 Name :Tat-CIRP peptide  
 Sequence :YGRKKRRQRRRGRGFSRGGGDRGYGG  
 Lot. No :MTFA30261-0705  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Shim-pack GIST C18(4.6\*250mm\*5um)  
 Dissolution method :100%H2O

Time	Module	Action	Value
0.01	Pumps	B.Conc	5
30.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	5
50.00	Controller	Stop	

### Chromatogram

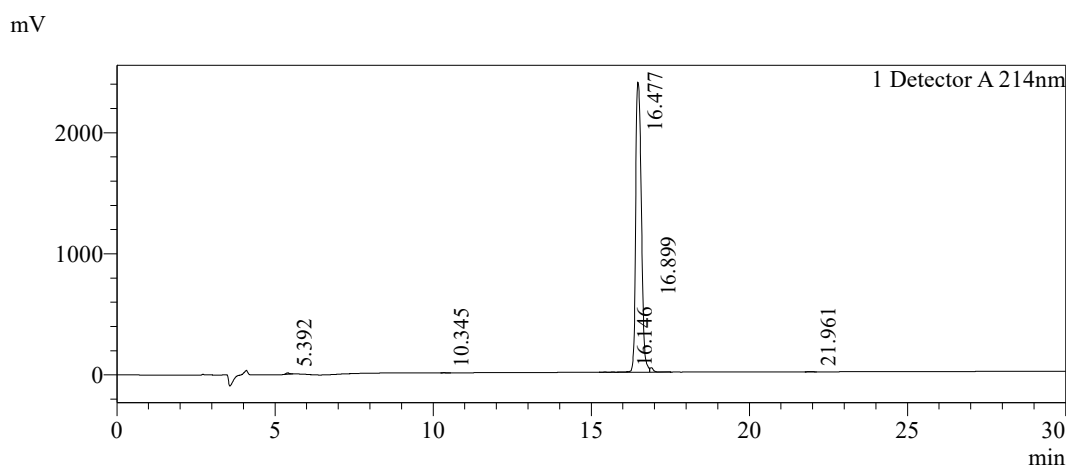


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	5.392	76626	11011	0.252
2	10.345	5071	773	0.017
3	16.146	79938	3710	0.263
4	16.477	29948593	2393270	98.470
5	16.899	294272	36785	0.968
6	21.961	9345	1056	0.031
Total		30413845	2446605	100.000

## MS Spectrum

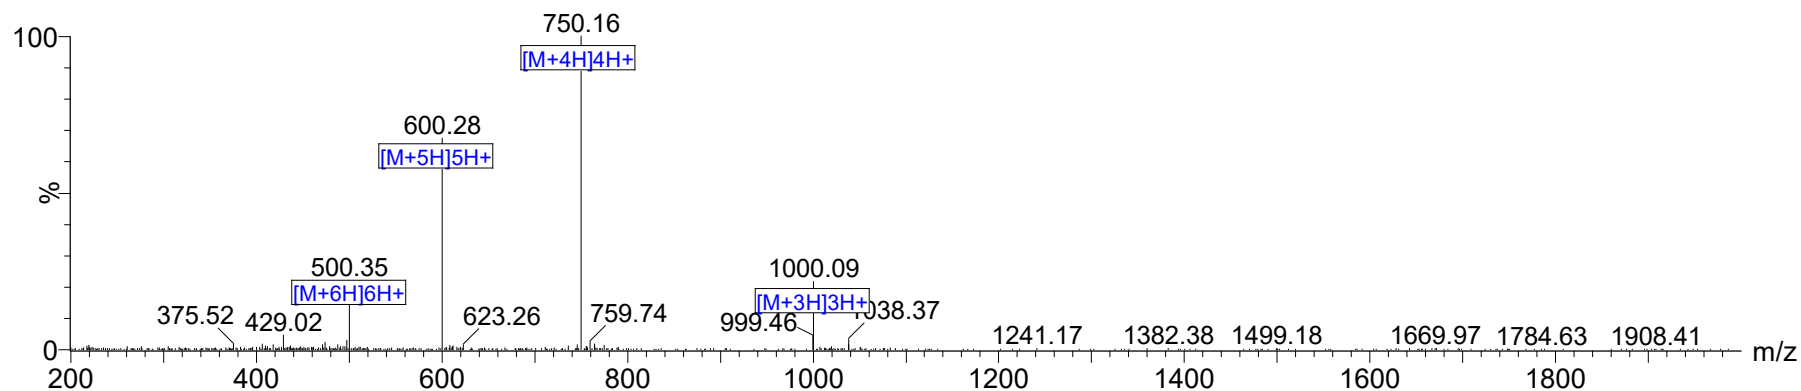 Positive  
Intensity


Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:7/20/2023 3:29:10	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID	: MTF30261
Name	: Tat-CIRP peptide
Sequence	: YGRKKRRQRRRGRGFSRGGGDRGYGG
Lot.No	: MTF30261-0705
Theoretical	: 2997.32
Observed	: 2996.64